


Lasers and Filters at the Class II NovoCyte Flow Cytometer

March 2021. Facs Core Facility, Aarhus University.

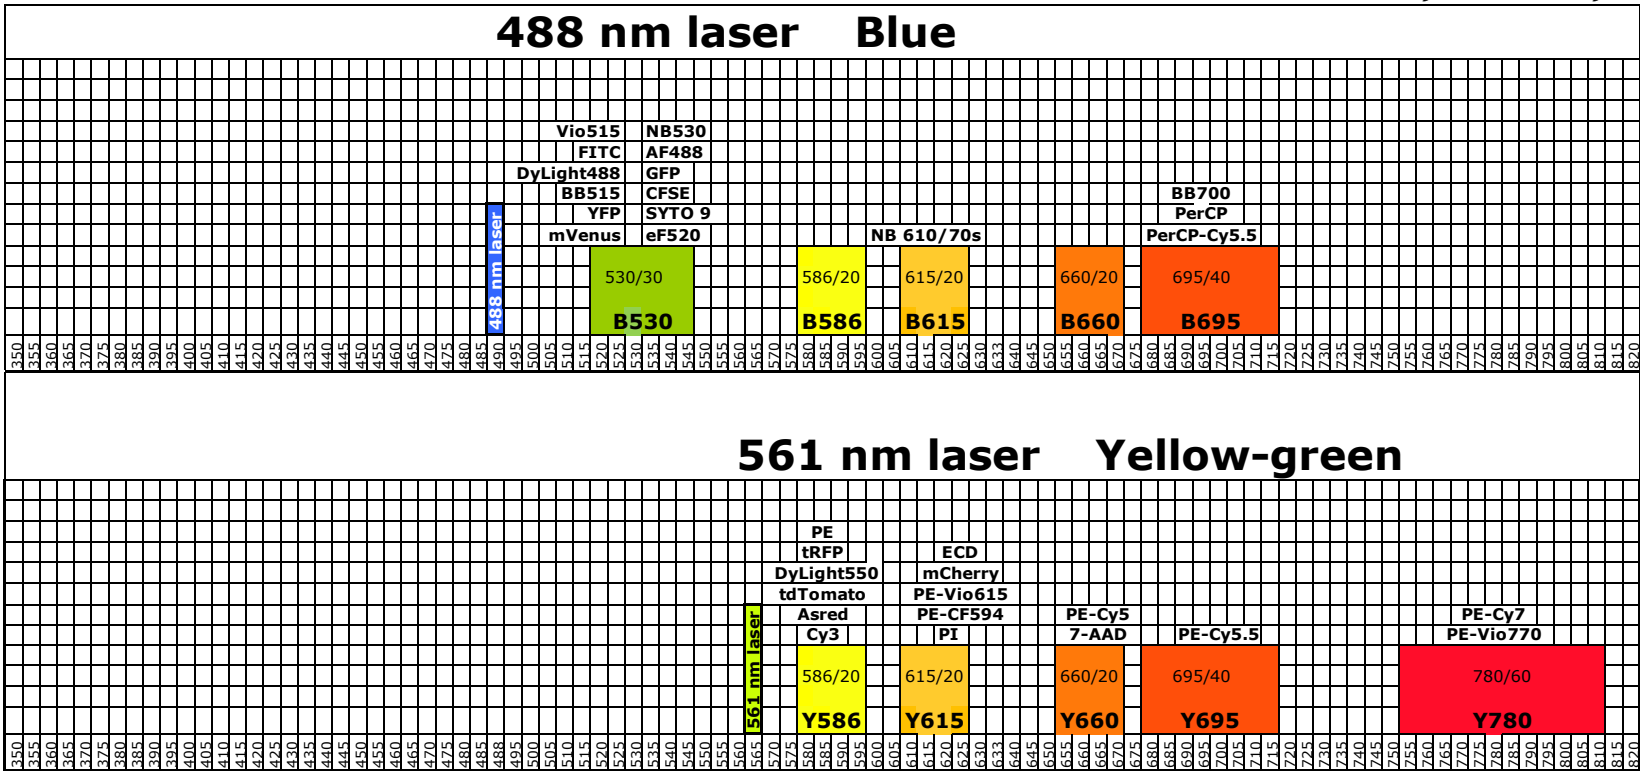

AF = Alexa Flour
 BV = Brilliant Violet
 eF = eFluor
 NB = Nova Blue
 BB = Brilliant Blue

Live dead dyes

Detector	Dye
B530	Live-or-dye 488/515 eFluor 520 Fix Viability Live/Dead Fix Scarlet Live/Dead Fix Green
Y586	Live-or-Dye 568/583
Y615	Live/Dead Fix Red
Y695	7AAD DRAQ7 Live-or-Dye 615/740